


# CERTIFICATE OF CALIBRATION

Date: 1/6/2015  
Model: 3525  
Serial Number:

Temperature: 74 °F  
Relative Humidity: 44 %

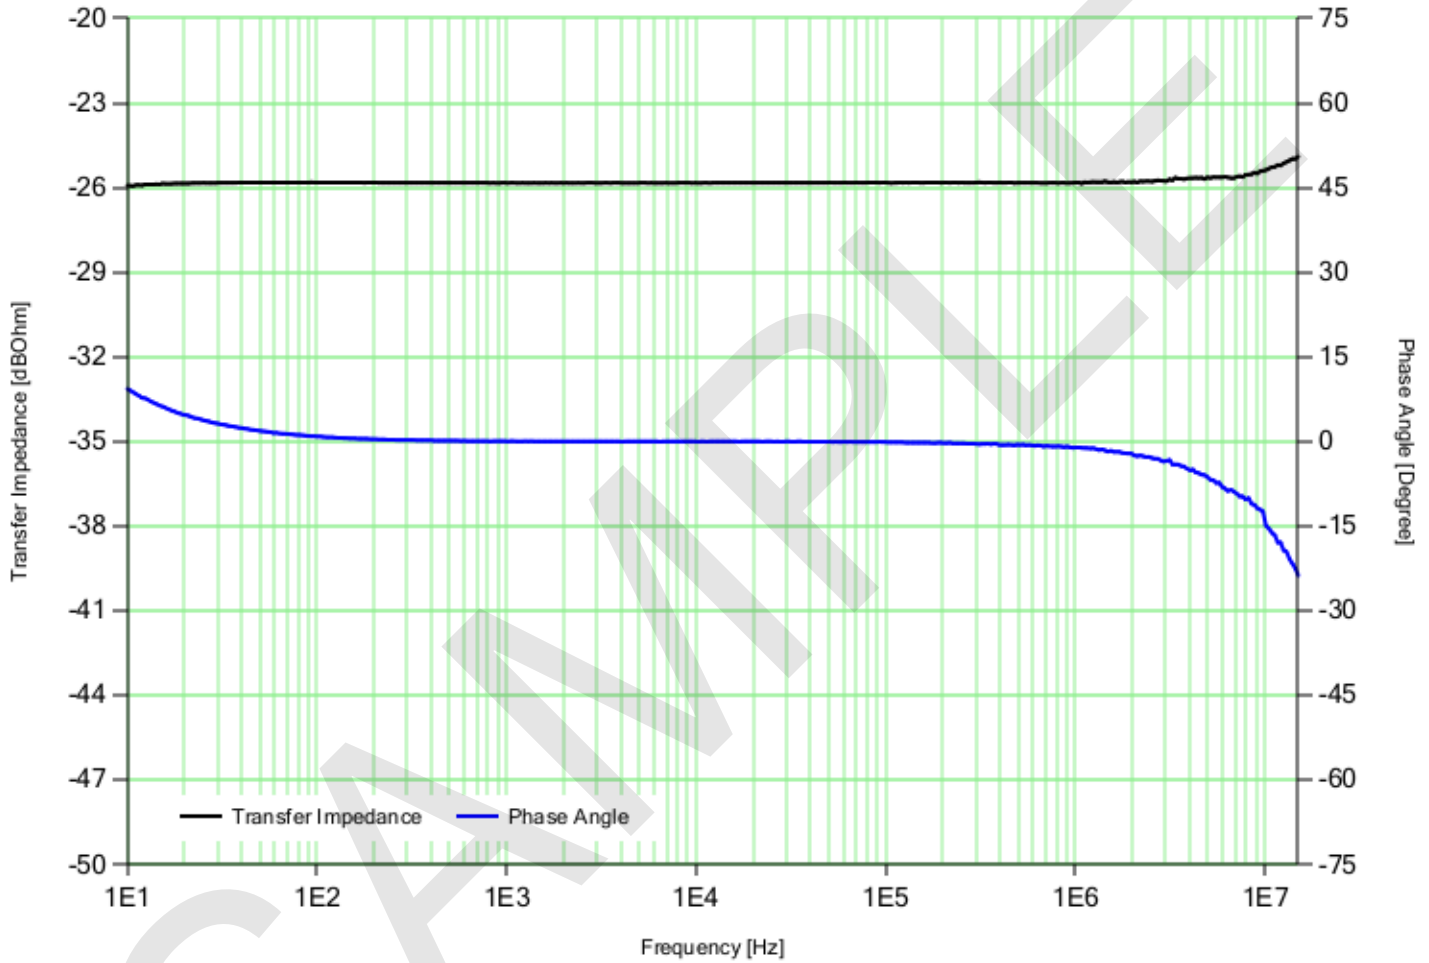

Nominal sensitivity 0.05(V/A) (-26 dB/Ohm)

The policies and procedures and this facility comply with ANSI/NCSL Z540-3 and ISO 9001:2008 and are traceable to NIST.

Calibration Equipment Used:

Model Type	ID Number	Cal Date	Due Date
HP 4195A Network Analyzer	2830J00997	09-21-14	09-21-16

Certified By: \_\_\_\_\_